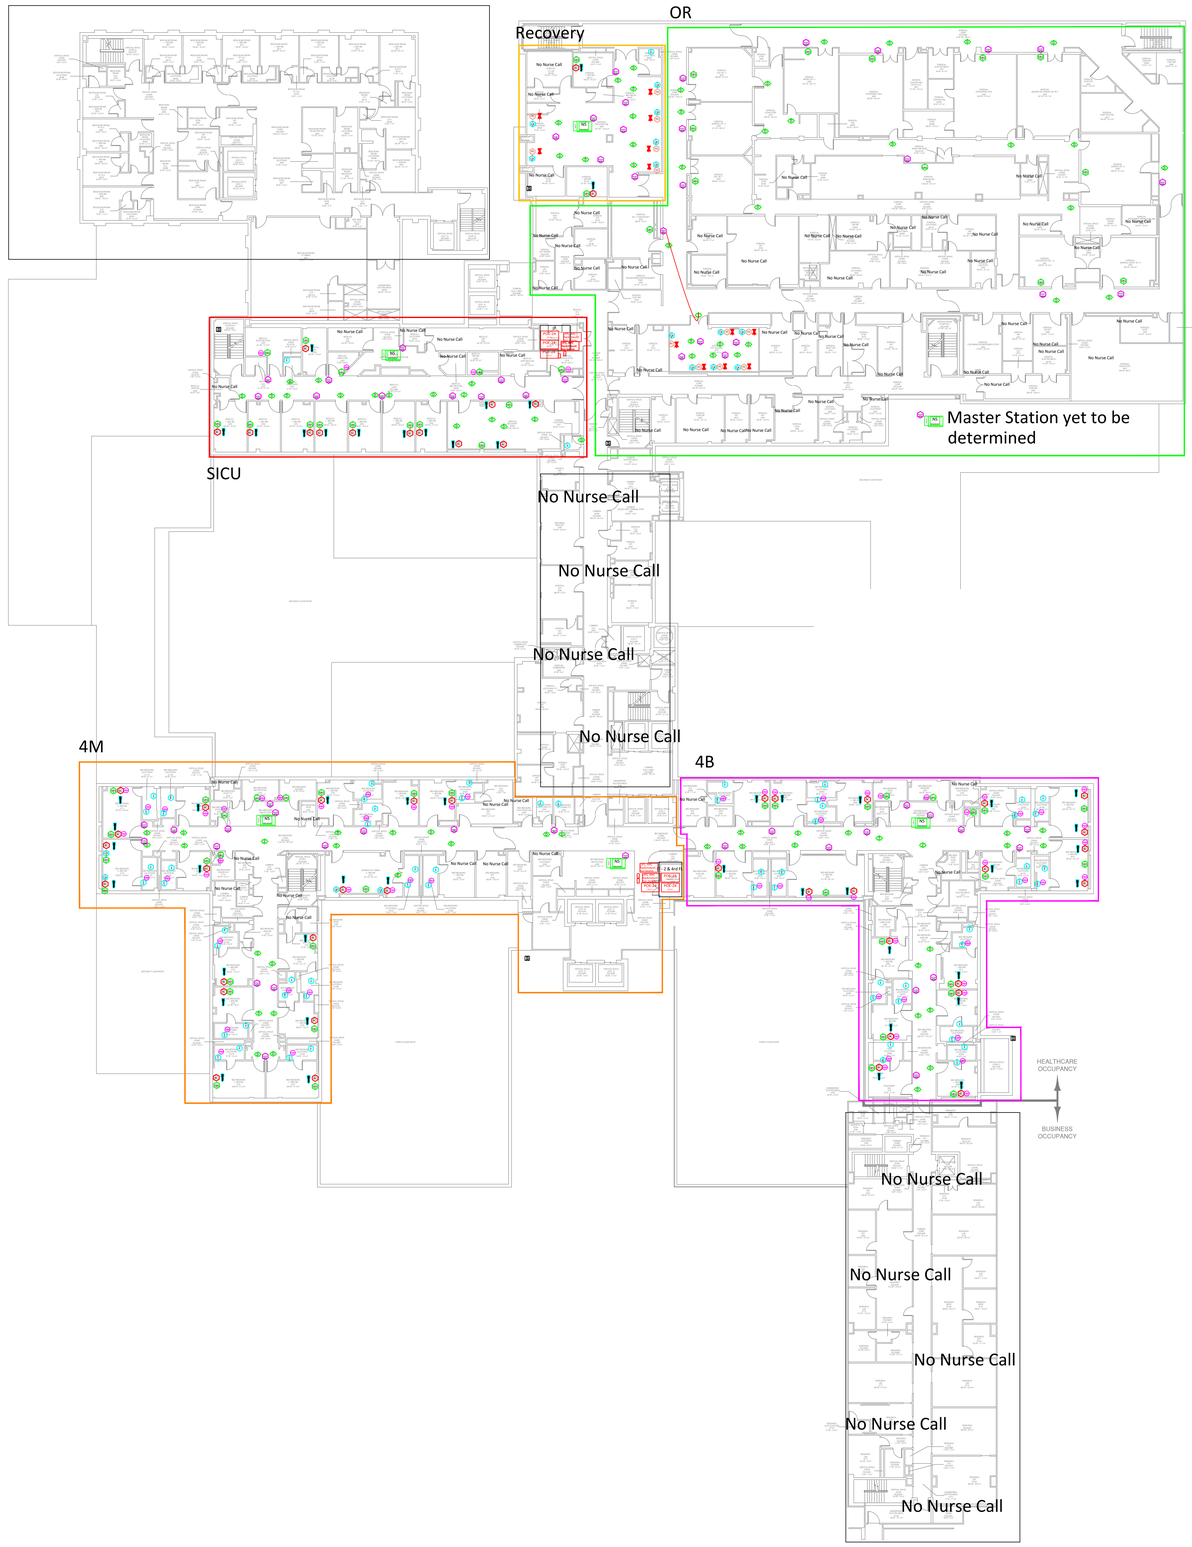

System Type = Hillrom CWS Unit: 4th FL 4M

5/16/2024	PNumber	QTY	Description
	AD18	4	INSTALLATION Audio Station (SRS, GRSS) Rough-in
	AD19	24	INSTALLATION Single-Gang Rough-in
NS	P2500VNC3C00	2	GRS10H DSK MNT, 4USB
	P2505NNC1C00	17	AUDIO STATION BED CONNECTOR
	P2506NNC3A02-G	19	DOME LIGHT, WHT -TAA COMPLIANT
	P2506NNC3A02-G	1	ZONE LIGHT, WHT -TAA COMPLIANT
	P25104C3312-Z105018	17	PILL SPK, DA,MIC,DV,N,2 L7.8'
POE-24	P2519NNC2A24	3	POE SWITCH NNC 24-PORT DELTA II
	P2519NNCFA00	2	MULTI MODE GBIC FOR HILL-ROM POE
	P2520NNC3A07	4	PB SWITCH, CODE BLUE, W/CANCEL
	P2520NNC3B01	17	PULL SWITCH,BATH W/CANCEL
	P2520NNC3B02	15	PULL SWITCH, BATH, W/O CANCEL
BATTERY BACKUP	P2521B02	2	UPS,RACKMOUNTABLE, 2U - NON-SEISMIC
	P2523C27	1	ADAPTER PLATE – DOME, 2G TO 1G
	P2594VNC1D01	4	STAFF STATION - STANDARD ROOM STATION W/O CODE
	P2594VNC1D11	16	PATIENT STATION - STANDARD ROOM STATION W/CODE
	P2599NNC3C00	15	RCB3 ROOM CONTROL BOARD

System Type = Hillrom CWS Unit: 4th FL 4B

5/16/2024	PNumber	QTY	Description
	AD18	3	INSTALLATION Audio Station (SRS, GRSS) Rough-in
	AD19	33	INSTALLATION Single-Gang Rough-in
NS	P2500VNC3C00	1	GRS10H DSK MNT, 4USB
	P2505NNC1C00	18	AUDIO STATION BED CONNECTOR
	P2506NNC3A02-G	16	DOME LIGHT, WHT -TAA COMPLIANT
	P2506NNC3A02-G	2	ZONE LIGHT, WHT -TAA COMPLIANT
	P25104C3312-Z105018	18	PILL SPK, DA,MIC,DV,N,2 L7.8'
	P2520NNC3B01	15	PULL SWITCH,BATH W/CANCEL
	P2520NNC3B02	15	PULL SWITCH, BATH, W/O CANCEL
	P2523C27	1	ADAPTER PLATE – DOME, 2G TO 1G
	P2594VNC1D01	3	STAFF STATION - STANDARD ROOM STATION W/O CODE
	P2594VNC1D11	15	PATIENT STATION - STANDARD ROOM STATION W/CODE
	P2599NNC3C00	12	RCB3 ROOM CONTROL BOARD

System Type = Hillrom CWS Unit: 4th FL SKY

5/16/2024	PNumber	QTY	Description
	AD18	4	INSTALLATION Audio Station (SRS, GRSS) Rough-in
NS	P2500VNC3C00	1	GRS10H DSK MNT, 4USB
	P2505NNC1C00	12	AUDIO STATION BED CONNECTOR
	P2506NSC3A02-G	15	DOME LIGHT, WHT -TAA COMPLIANT
	P2506NSC3A02-G	1	ZONE LIGHT, WHT -TAA COMPLIANT
	P25104C3312-Z105018	12	PILL SPK, DA,MIC,DV,N,2 L7.8'
POE-24	P2519NNC2A24	3	POE SWITCH NNC 24-PORT DELTA II
	P2519NNCFA00	2	MULTI MODE GBIC FOR HILL-ROM POE
	P2520NNC3B01	2	PULL SWITCH,BATH W/CANCEL
BATTERY BACKUP	P2521B02	3	UPS,RACKMOUNTABLE, 2U - NON-SEISMIC
	P2523C27	1	ADAPTER PLATE – DOME, 2G TO 1G
	P2594VNC1D01	4	STAFF STATION - STANDARD ROOM STATION W/O CODE
	P2594VNC1D11	10	PATIENT STATION - STANDARD ROOM STATION W/CODE
	P2599NNC3C00	11	RCB3 ROOM CONTROL BOARD

System Type = Hillrom CWS Unit: 4th FL Recovery

5/16/2024	PNumber	QTY	Description
NS	P2500VNC3C00	1	GRS10H DSK MNT, 4USB
	P2505NNC1C00	2	AUDIO STATION BED CONNECTOR
	P2506NNC3A02-G	9	DOME LIGHT, WHT -TAA COMPLIANT
	P25104C3310-Z105018	2	PILL SPK, DA,MIC,DV,N,2 L7.8'
	P2511SOC-0101-080-U	6	CALL CORD, OXYGEN SAFE, 8 FT
	P2516A01	6	EQUIPMENT RECEPTACLE
	P2520NNC3A07	6	PB SWITCH, CODE BLUE, W/CANCEL
	P2520NNC3B01	1	PULL SWITCH,BATH W/CANCEL
	P2523C27	1	ADAPTER PLATE – DOME, 2G TO 1G
	P2594VNC1D11	2	PATIENT STATION - STANDARD ROOM STATION W/CODE
	P2599NNC3C00	7	RCB3 ROOM CONTROL BOARD

System Type = Hillrom CWS Unit: 4th FL OR

5/16/2024	PNumber	QTY	Description
NS	P2500VNC3C00	1	GRS10H DSK MNT, 4USB
	P2506NNC3A02-G	25	DOME LIGHT, WHT -TAA COMPLIANT
	P2506NNC3A02-G	1	ZONE LIGHT, WHT -TAA COMPLIANT
	P2511SOC-0101-080-U	6	CALL CORD, OXYGEN SAFE, 8 FT
	P2516A01	6	EQUIPMENT RECEPTACLE
	P2520NNC3A07	6	PB SWITCH, CODE BLUE, W/CANCEL
	P2523C27	1	ADAPTER PLATE – DOME, 2G TO 1G
	P2594VNC1D01	1	STAFF STATION - STANDARD ROOM STATION W/O CODE
	P2594VNC1D11	11	PATIENT STATION - STANDARD ROOM STATION W/CODE
	P2599NNC3C00	17	RCB3 ROOM CONTROL BOARD

PRELIMINARY
DRAWING ONLY
12/07/2023
DO NOT USE FOR CONSTRUCTION

DRAWN BY: LPK
CHECKED BY:

N

NOTICE
The drawings and all information thereon is property of:
BAXTER HEALTHCARE CORPORATION
BATESVILLE, INDIANA
This drawing and information thereon, is confidential and must not be made public, copied, or used to disadvantage of said Baxter Healthcare Corporation
The drawing and all information is subject to return to Baxter on demand.

BAXTER
NURSE CALL SOLUTIONS
1225 CRESCENT GREEN
SUITE 200
CARY, NC 27518
www.hillrom.com

Hillrom™
Hillrom is a part of Baxter

Revision Date	Revised by	Comments

Revision History

Drawing Information
03 DWG QWAQ15097-01 VAMC 521 BIRMINGHAM 4TH FLOOR.dwg
Sheet Number: 4
Total Sheets: 12
Drawing Scale: 1" = 20'
U.L. LISTED

Project Information
REPLACE NURSE CALL SYSTEM
Proposal #QWAQ15097-02
NURSE CALL LAYOUT

Customer Information
610128
VETERANS AFFAIR MEDICAL CENTER 521
700 19TH ST S
BIRMINGHAM AL 352331927