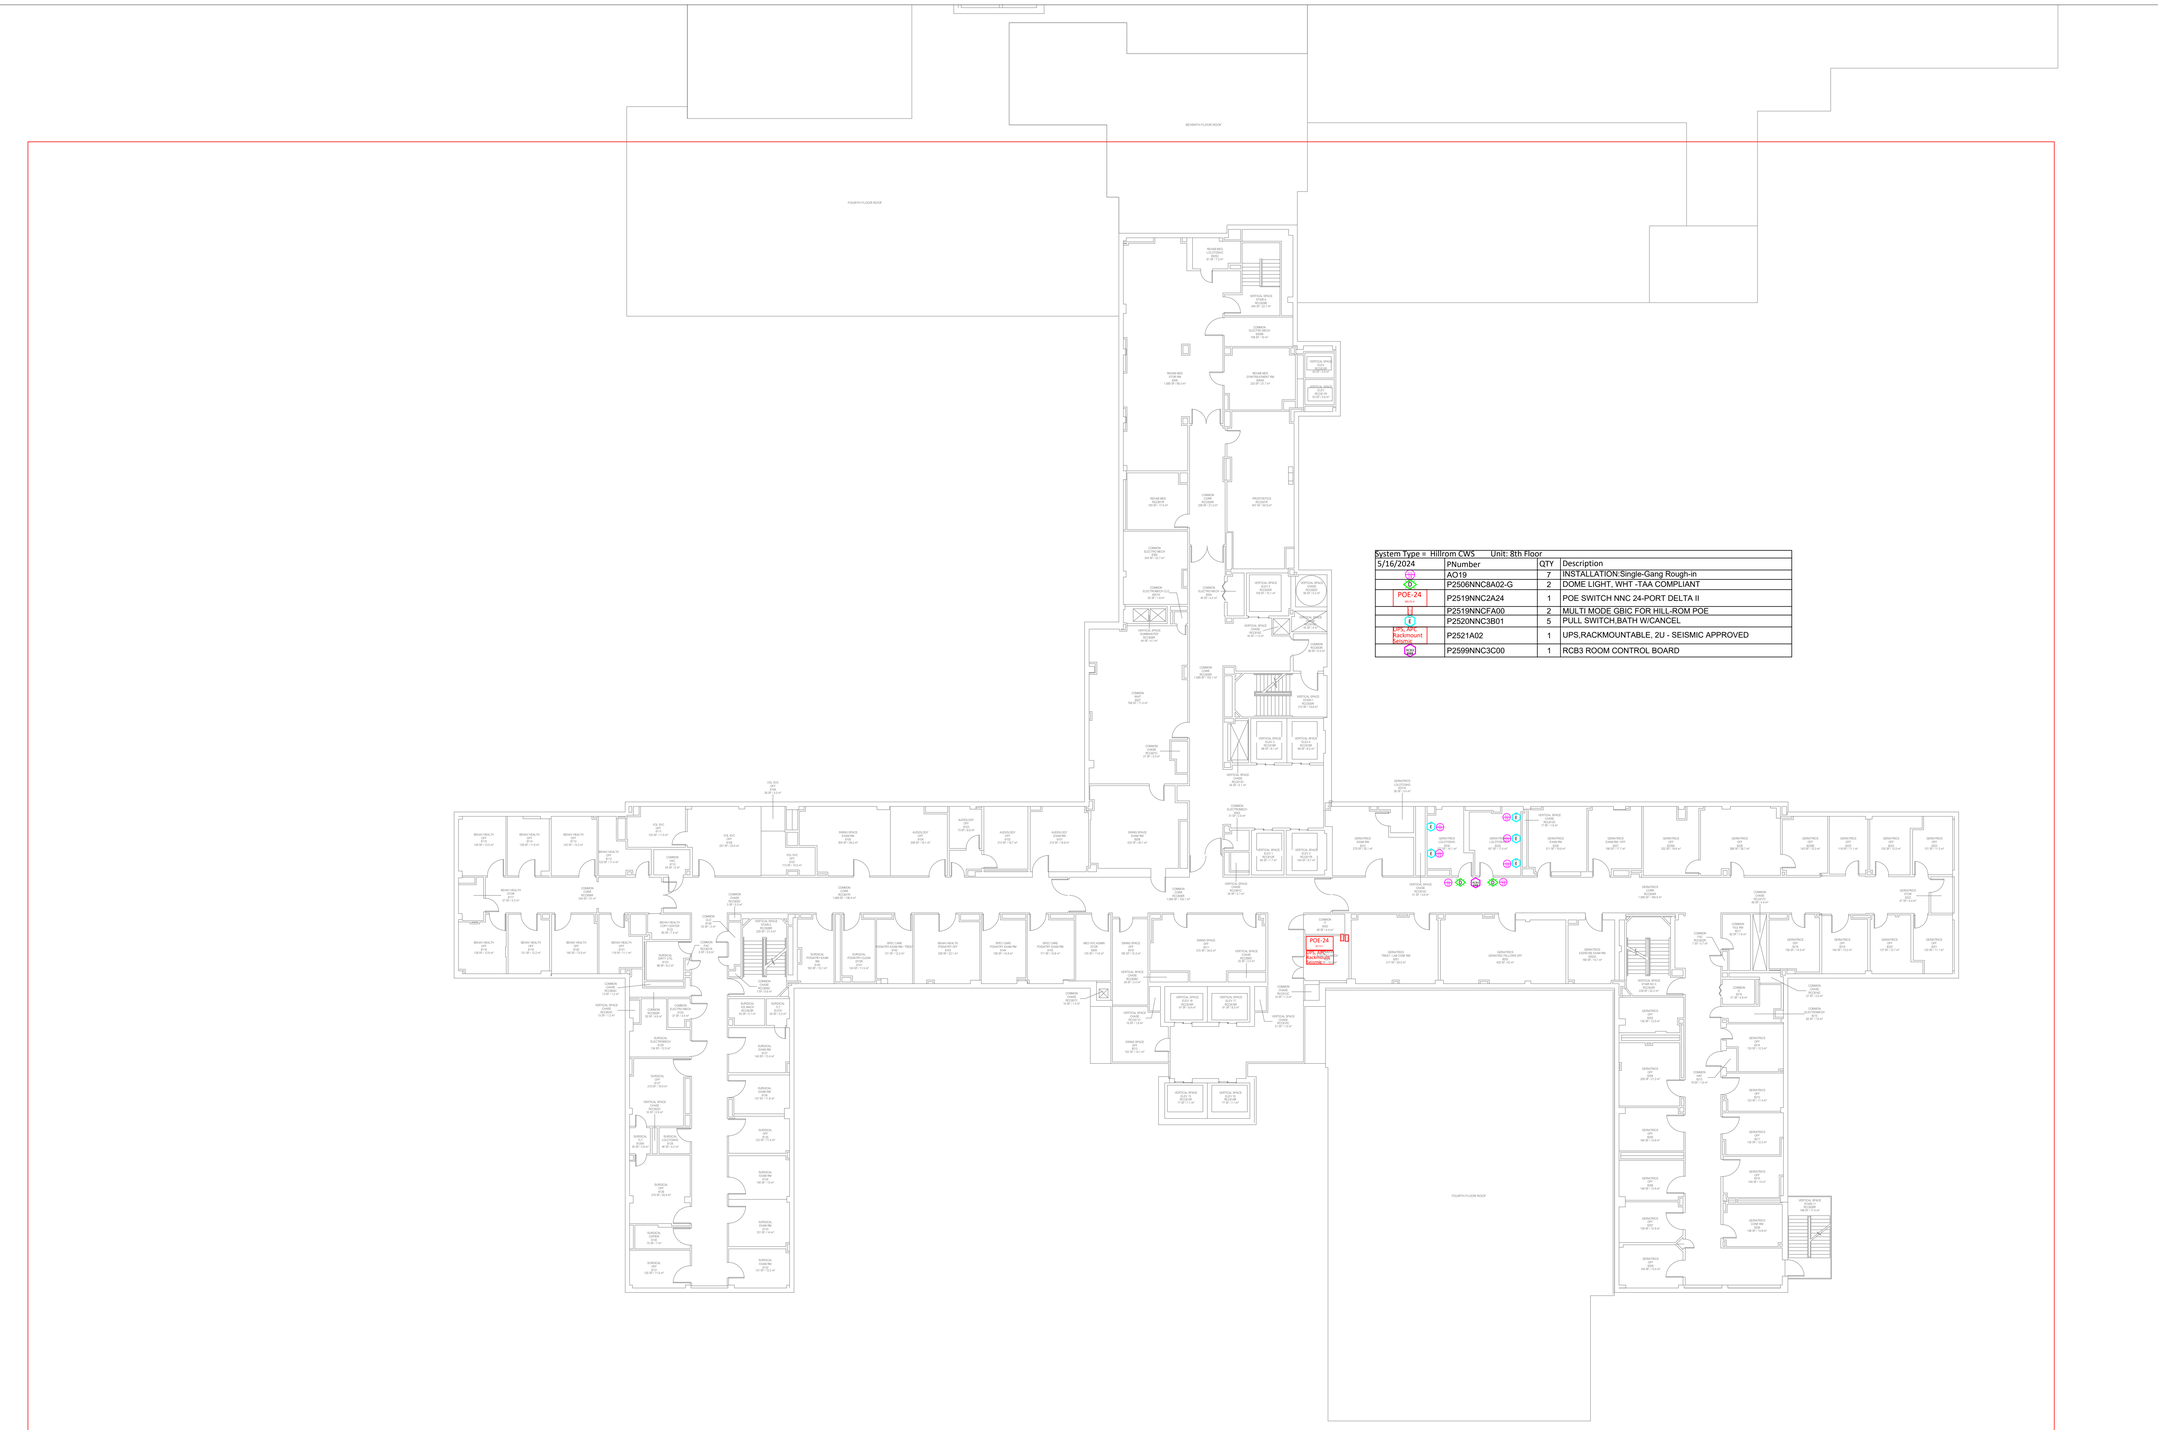


System Type = Hillrom CWS Unit: 8th Floor

| 5/16/2024 | PNumber | QTY | Description |
|---|---|---|---|
| AO19 | AO19 | 7 | INSTALLATION:Single-Gang Rough-in |
| | P2506NNC8A02-G | 2 | DOME LIGHT, WHT -TAA COMPLIANT |
| POE-24 | P2519NNC2A24 | 1 | POE SWITCH NNC 24-PORT DELTA II |
| | P2519NNCFA90 | 2 | MULTI MODE GBIC FOR HILL-ROM POE |
| E | P2520NNC3B01 | 5 | PULL SWITCH,BATH W/CANCEL |
| UPS, APS, Rackmount, SEISMIC | P2521A02 | 1 | UPS,RACKMOUNTABLE, 2U - SEISMIC APPROVED |
| RCB3 | P2599NNC3C00 | 1 | RCB3 ROOM CONTROL BOARD |

N

NOTICE
The drawings and all information thereon is property of:
BAXTER HEALTHCARE CORPORATION
BATESVILLE, INDIANA
This drawing and information thereon, is confidential and must not be made public, copied. or used to disadvantage of said Baxter Healthcare Corporation
The drawing and all information is subject to return to Baxter on demand.

BAXTER
NURSE CALL SOLUTIONS
1225 CRESCENT GREEN
SUITE 200
CARY, NC 27518
www.hillrom.com

Hillrom™
Hillrom is a part of Baxter

| Revision Date | Revised by | Comments |
|---|---|---|
| | | |

Revision History

Drawing Information
10 DWG QWAQ15097-02 VAMC 521 BIRMINGHAM 8TH FLOOR.dwg
Sheet Number 11
Total Sheets 12
Drawing Scale 1" = 20'
U.L. LISTED

Project Information
REPLACE NURSE CALL SYSTEM
Proposal #QWAQ15097-02
NURSE CALL LAYOUT

Customer Information
610128
VETERANS AFFAIR MEDICAL CENTER 521
700 19TH ST S
BIRMINGHAM AL 352331927