
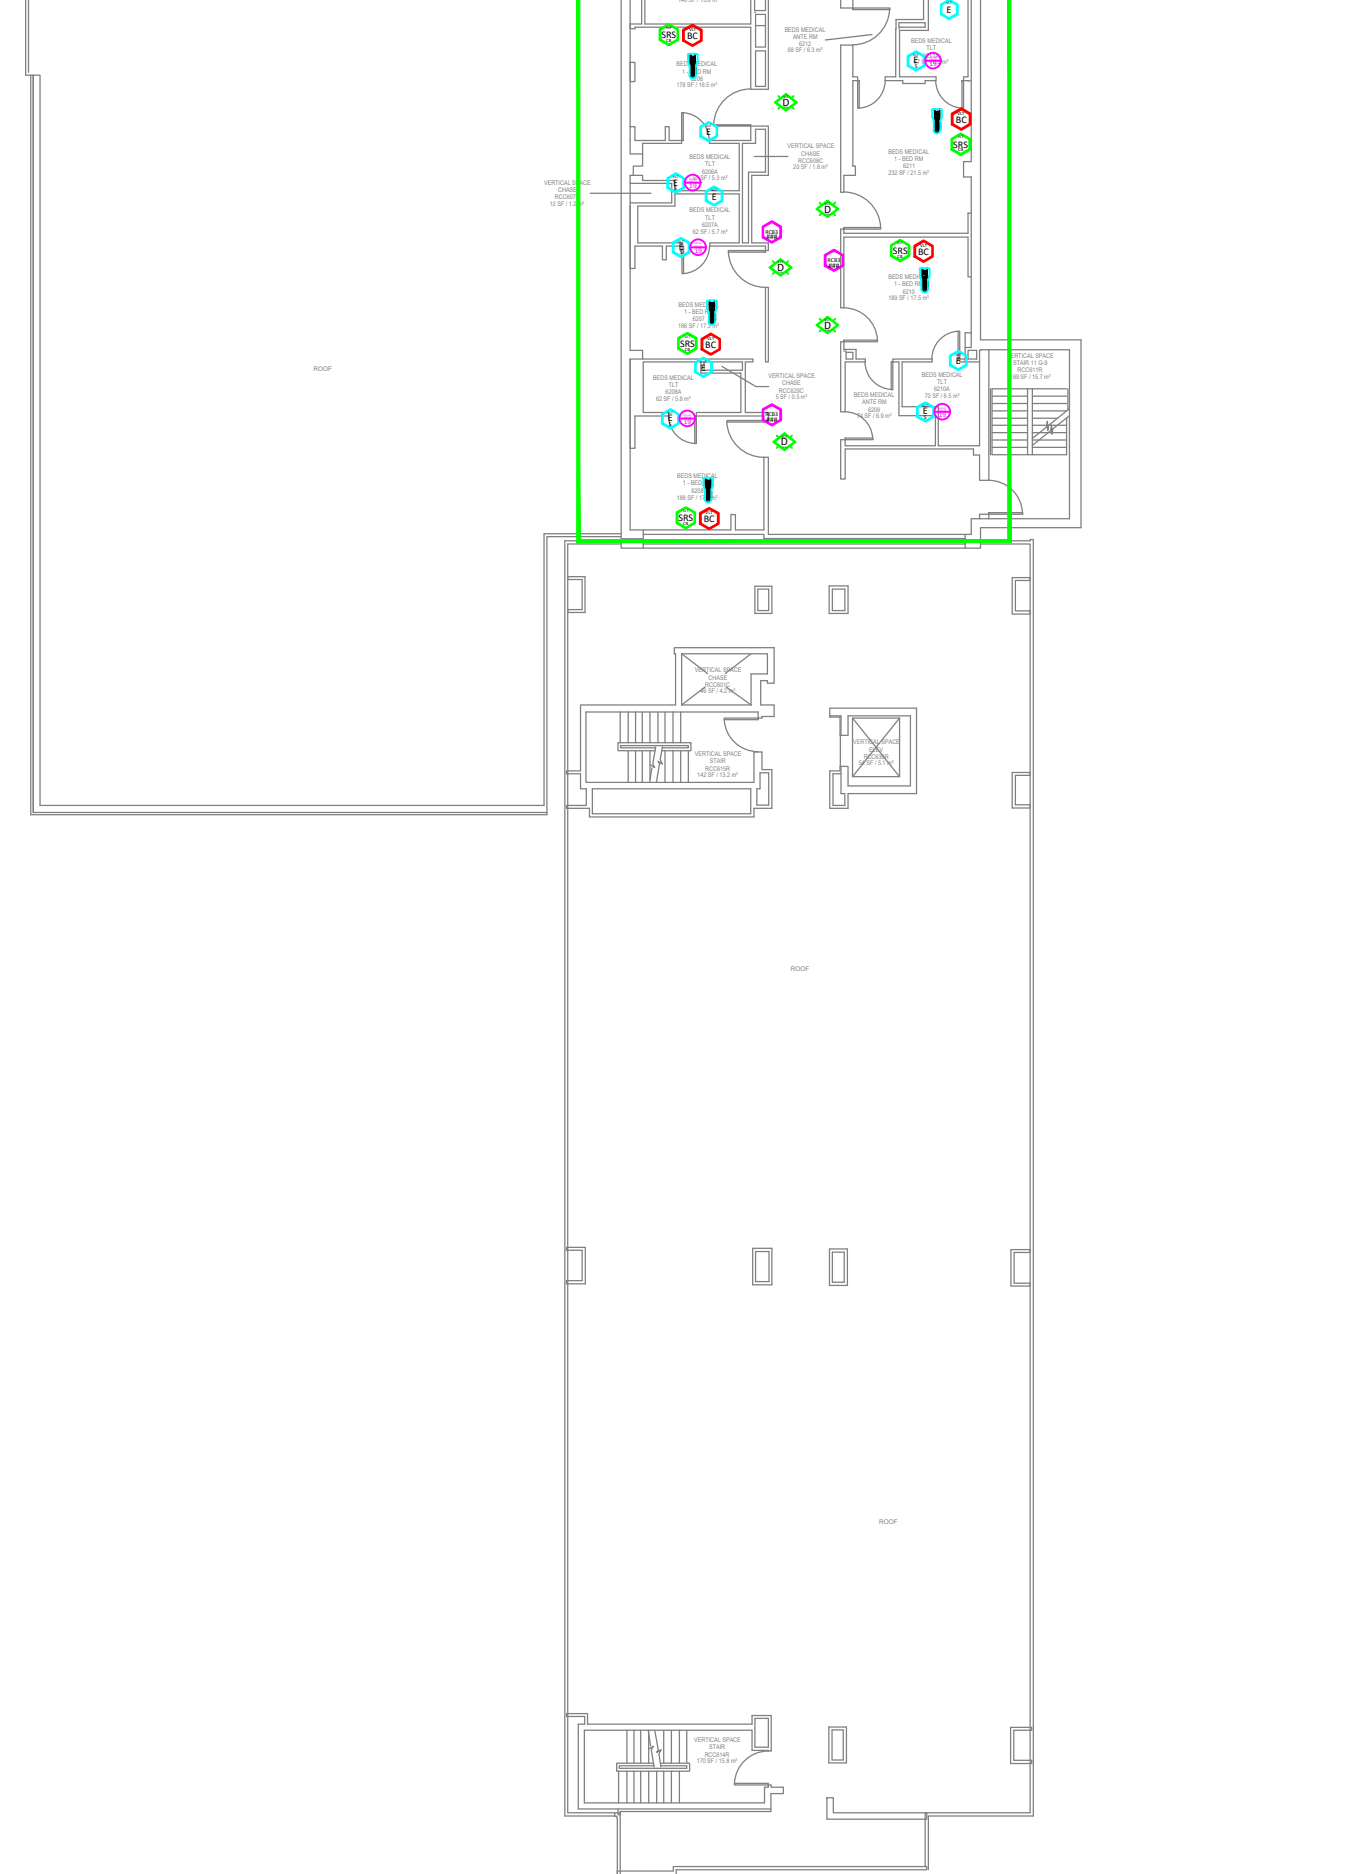
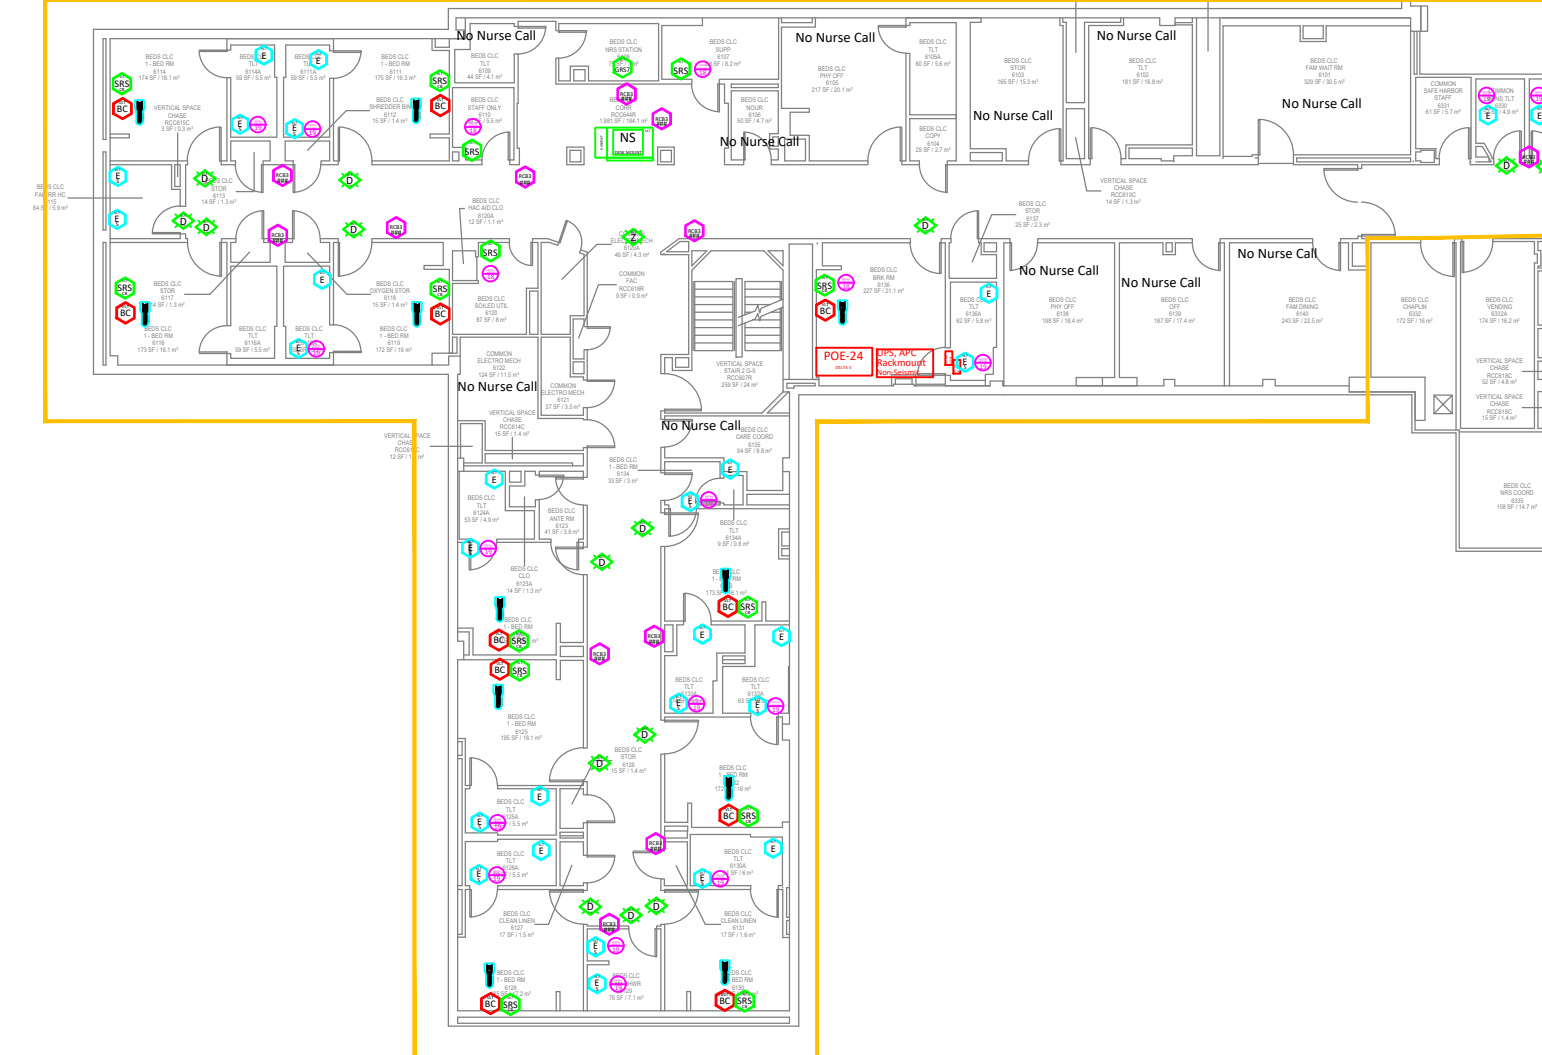
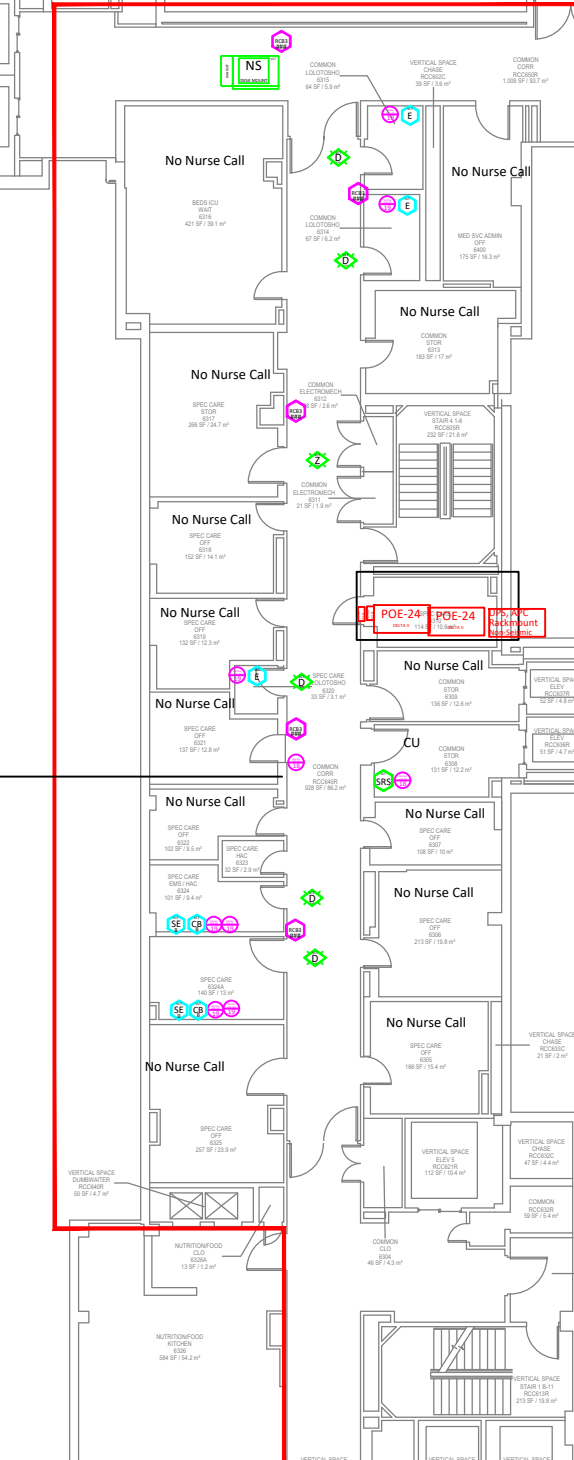
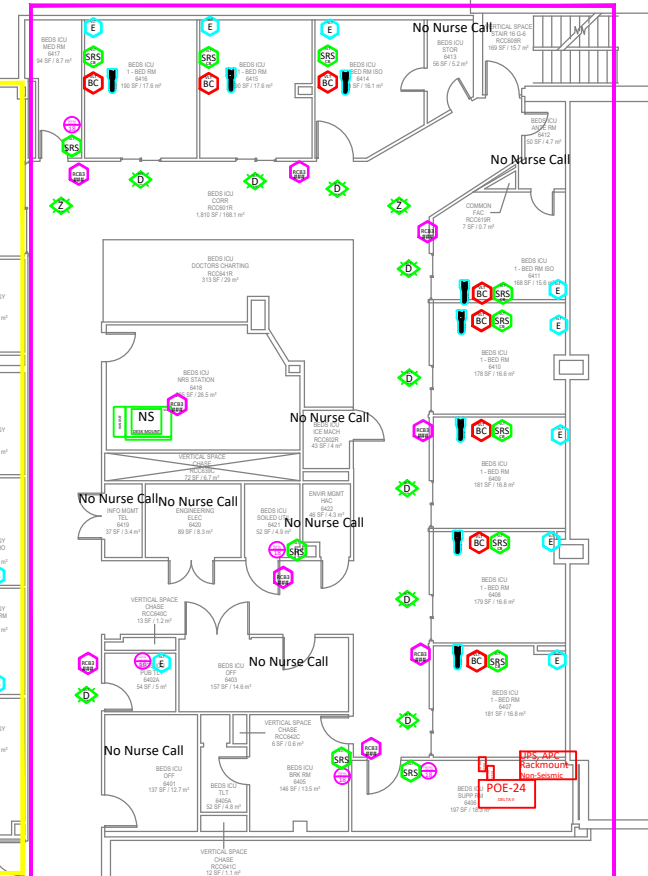
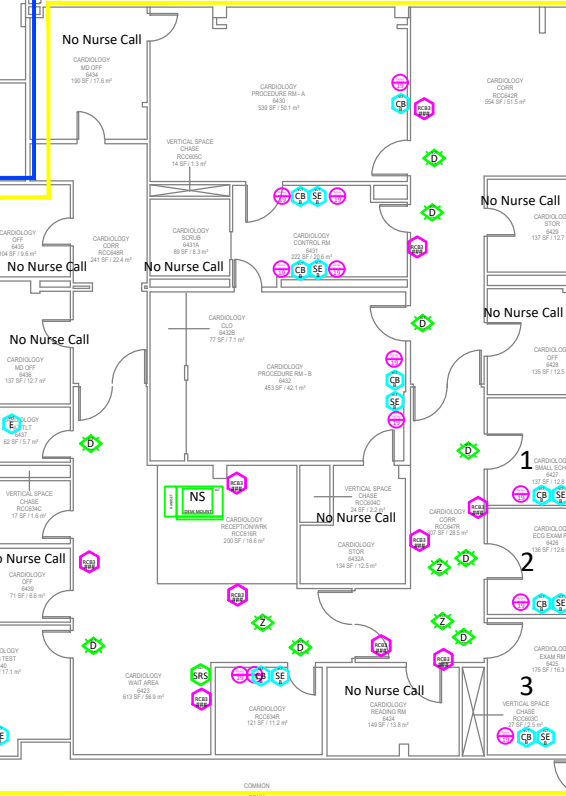


[illegible]

System Type	Person	Unit Ref	MV	Description
5/16/2014	Phumber	AZ08	1	INSTATION/Audio Station (BRS, GRSS) Roughin
	NS	P595NNWC00	1	NOISE GSK MNT. AUBH
	NS	P595NNC100	1	AUTO STATION/DC CONNECTOR
	NS	P595NNCA02.G	1	DOME LIGHT -WAT-TAN CLAMP#
	FOR-24	P510AC231U-2105018	10	PILL BOX, DMG DMC-HV N.2 L.17.8"
	NS	P510NNA2A24	1	POE SWITCH/STK 24-POR. PORT. DIA II
	NS	P510NNA2000	1	MULTI MODE DSX FOR HIL-DOMA FIO
	NS	P595NNWC001	1	FLEX-SOUND BATH INCHANCE
	NS	P5021R02	1	UPS/RECOUNTABLE-BATT. 3. NON-SEISMIC
	NS	P595NNC1001	4	STAFF STATION - STANDARD ROOM STATION W/O CODE
	NS	P595NNC111	10	PATIENT STATION - STANDARD ROOM STATION W/CODE
	NS	P595NNCC00	10	R03 ROOM CONTROL BOARD

[illegible]

System Type = HFCOM-450		Unit: 400k BTU/h		Circuitology	
		Plumber	QTY	Description	
		AO19	16	INSTALLATION Single-Gang Roogheen	
		G/5160VNC3C00	1	G/516 10 DSK MNT. 4U58	
		P2560VNC3A02-G	9	ZONE LIGHT, WH/ T-XXA COMPLANT	
		P2560VNC3A02-G	9	ZONE LIGHT, WH/ T-XXA COMPLANT	
		P2560VNC3A07	9	SW SWITCH, COLO BLUE, INWANGEL	
		P2560VNC3A08	9	PU SW/ITCH STAGE EMER INWANGEL	
		P2560VNC3B01	8	PULL SWITCH/UBATH WICANGEL	
		P2564VNC1D01	1	STAFF STATION - STANDARD ROOM STATION W/ CODE	
		P2566VNC3A00	10	RCB3 ROOM CONTROL BOARD	

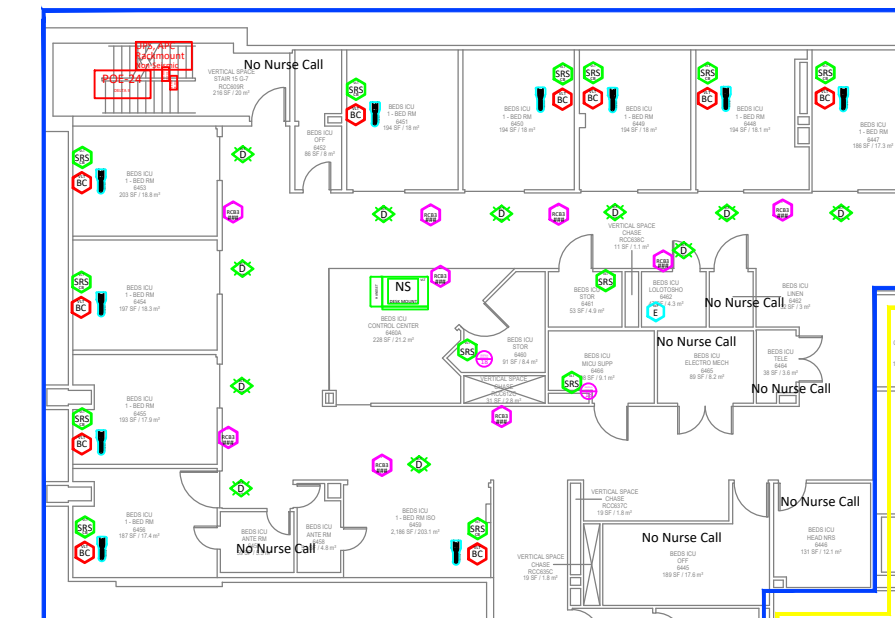

Hillrom is a part of Baxter

Revision Date	Revised by	Comments
Revision History:		

U.L. LISTED

Project Information
REPLACE NURSE CALL SYSTEM
Proposal #QWAQ15097-02
NURSE CALL LAYOUT

<u>Customer Information</u>			
610128			
VETERANS AFFAIR MEDICAL CENTER 521			
700 19TH ST S			
BIRMINGHAM		AL	352331927